



ZPure™ PolyGas I Purifiers with Compression Fittings





Warnings

Warnings must be read carefully and understood. Improper use of this product can cause harm or death to personnel and damage to property!



Wear eye protection and use caution when working with pressurized systems.

Maximum pressure rating is noted in table below.

When using a high-pressure gas source overpressure protection must be provided.

Do not open filter, even after use.


The rapid oxidation of the active adsorbent in this filter can cause the filter bed to become hot. Limited exposure of the filter to air during installation does not result in rapid reaction or dangerous heat generation.

Do not use with supply gas H₂O concentration or O₂ concentration greater than 0.1%. Contains molecular sieve which may become very hot in contact with liquid water. Do not use with liquids.

Special precautions might be required when using hydrogen or hazardous gases. Consult local regulations and your company's safety procedures.

Product Numbers

Size	1/8" Brass	1/4" Brass	1/8" SS	1/4" SS	Maximum Pressure
130 cc	202285-B	202286-B	202285-SS	202286-SS	68.9 bar / 1000 psi
475 cc	202285L-B	202286L-B	202285L-SS	202286L-SS	68.9 bar / 1000 psi
500 cc	202285D-B	202286D-B	202285D-SS	202286D-SS	13.8 bar / 200 psi
750 cc	202285XL-B	202286XL-B	202285XL-SS	202286XL-SS	13.8 bar / 200 psi

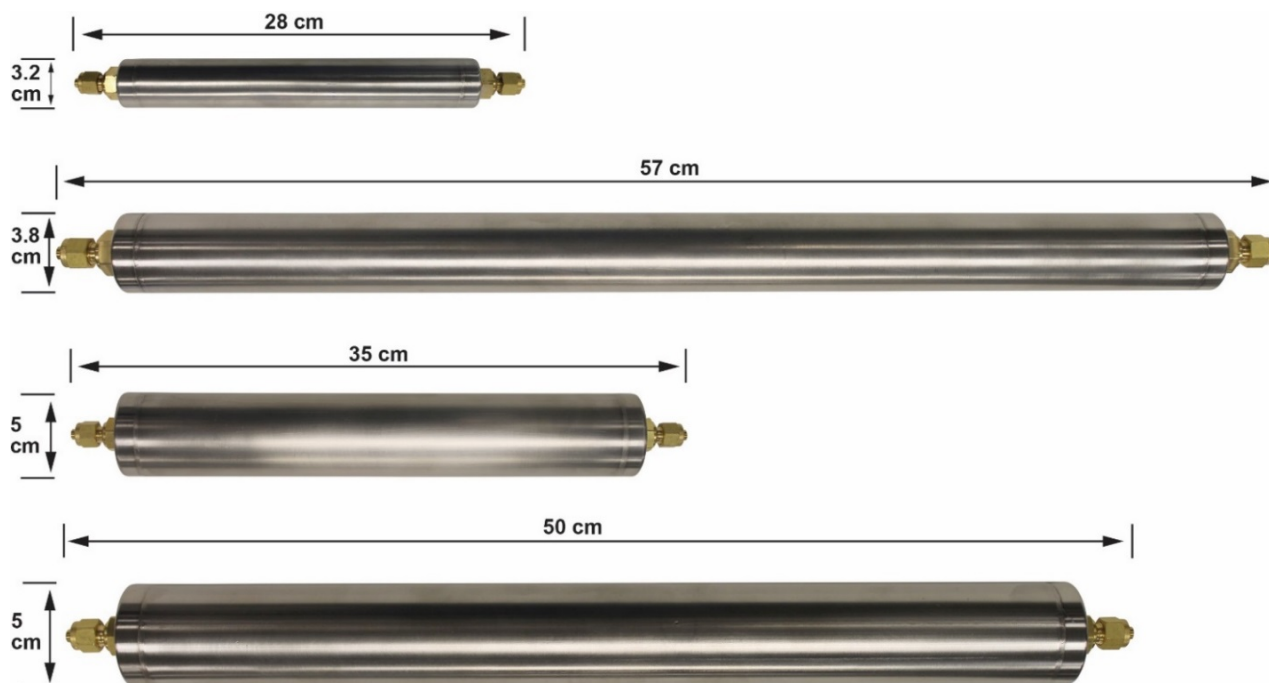

From top to bottom: 130 cc, 475 cc, 500 cc, 750 cc

Filter Setup and Use

Installation for Compression Fittings

1. Check the package contents for damage. Contact your supplier if any items are damaged or missing.
2. The ZPure Filter is delivered in the active state, filled with helium. It is ready for use, but it is recommended that the trap be purged with the gas to be purified.
3. For the best connections, start with freshly-cut tubing in the gas line. 1/8" nuts should be turned 3/4 turn past finger tight. 1/4" nuts should be turned 1-1/4 turns past finger tight.
4. To connect in-line, first purge the gas line with the supply gas. While maintaining a low purge rate of 10 to 30 cc/min, remove the end plugs from both ends of the trap, then attach the inlet end of the trap to the gas line.
5. While the end plugs are removed from the trap during installation, a small amount of air will diffuse into the adsorbent. As long as the trap is attached to the gas line within a few minutes, the loss of adsorbing capacity will be negligible.
6. Attach the outlet end of the trap.
7. Purge the entire system until a total of 1 to 2 liters of gas has been flushed through.
8. Leak check all connections.



Trajan Scientific Americas Inc
2601 Technology Drive,
Louisville, KY 40299, USA
Tel: 502 491 6300
Fax: 502 491 3390
usa@trajanscimed.com



Recycling

Please contact CRS for information regarding recycling and reconditioning gas purifier products.