


## ZPure™ O<sub>2</sub>/H<sub>2</sub>O filters

### Quick connect fittings

#### Introduction

Pure gas is critical requirement in gas chromatography, spectroscopy, optics, lithography, and numerous other applications in manufacturing and analytical laboratories. The ZPure™ O<sub>2</sub>/H<sub>2</sub>O filters remove O<sub>2</sub> and H<sub>2</sub>O from inert gases, He, Ar, N<sub>2</sub>, H<sub>2</sub>, making it ideal for use with GC and GC/MS carrier gas lines.

It is also recommended for any application requiring ultra-pure gas free from oxygen and moisture.

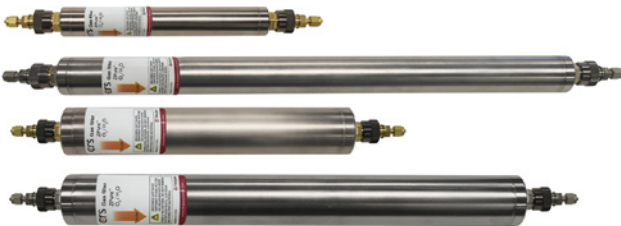

#### Important



Warnings must be read carefully and understood. Improper use of this product can cause harm or death to personnel and damage to property!

- Wear eye protection and use caution when working with pressurized systems.
- Maximum pressure is 13.8 bar / 200 psi.
- When using a high-pressure gas source over-pressure protection must be provided.
- Do not open filter, even after use.
- The rapid oxidation of the active adsorbent in this filter can cause the filter bed to become extremely hot, resulting in danger of fire or burn injuries. Limited exposure of the filter to air during installation does not result in rapid reaction or dangerous heat generation.

- Do not pass air or oxidizing gases in concentration above 0.1% through this filter!
- Special precautions might be required when using hydrogen or hazardous gases. Consult local regulations and your company's safety procedures.

#### Instructions

##### Installation for quick connect fittings

1. Check the package contents for damage. Contact your supplier if any items are damaged or missing.
2. The filters are delivered in the active state, filled with helium. It is ready for use, but it is recommended that the trap be purged with the gas to be purified.
3. Install the quick connect tube fittings ends to the gas lines. For the best connections, start with freshly-cut tubing in the gas line. 1/8" nuts should be turned 3/4 turn past finger tight. 1/4" nuts should be turned 1-1/4 turns past finger tight.
4. Attach the outlet end of the filter by screwing the quick connect fitting nut onto the adapter. This will open both check valves on the outlet side.
5. Attach the inlet end of the filter by screwing the quick connect fitting nut onto the adapter. This will open the check valves in both the quick connect tube fitting and the quick connect adapter, allowing gas to flow through.
6. Purge the entire system until a total of 1 to 2 liters of gas has been flushed through.
7. Leak check all connections.

### Specifications

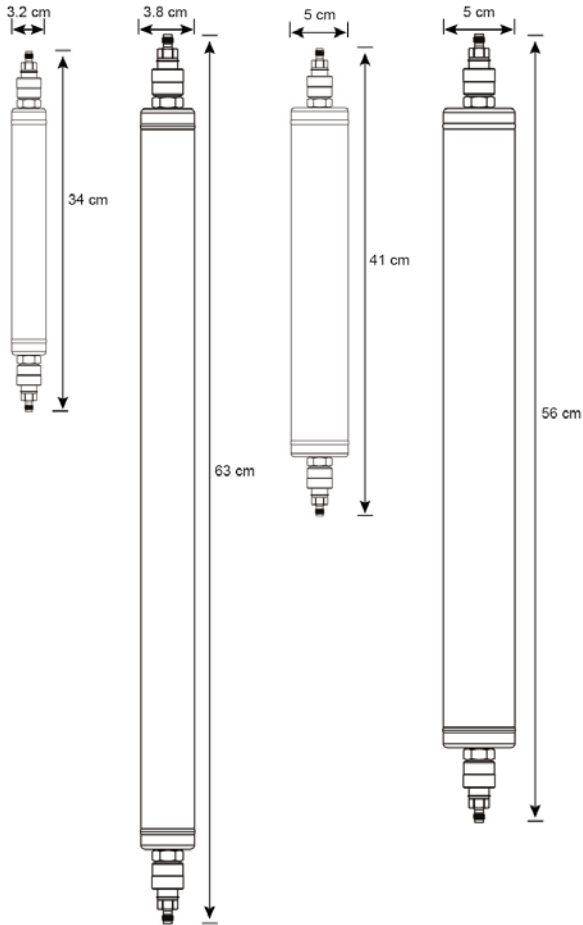


Figure 1. From left to right: 130 cc, 475 cc, 500 cc, 750 cc

### Product numbers

130 cc	
1/8" Brass	1/4" Brass
202295-B-QC	202296-B-QC
1/8" Stainless steel	1/4" Stainless steel
202295-SS-QC	202296-SS-QC
475 cc	
1/8" Brass	1/4" Brass
202295L-B-QC	202296L-B-QC
1/8" Stainless steel	1/4" Stainless steel
202295L-SS-QC	202296L-SS-QC
500 cc	
1/8" Brass	1/4" Brass
202295D-B-QC	202296D-B-QC
1/8" Stainless steel	1/4" Stainless steel
202295D-SS-QC	202296D-SS-QC

750 cc	
1/8" Brass	1/4" Brass
202295XL-B-QC	202296XL-B-QC
1/8" Stainless steel	1/4" Stainless steel
202295XL-SS-QC	202296XL-SS-QC
Replacement cartridge	
130 cc	
Brass	Stainless steel
202ROH-B-QC	202ROH-SS-QC
475 cc	
Brass	Stainless steel
202ROHL-B-QC	202ROHL-SS-QC
500 cc	
Brass	Stainless steel
202ROHD-B-QCB	202ROHD-SS-QC
750 cc	
Brass	Stainless steel
202ROHXL-B-QC	202ROHXL-SS-QC

### References



#### Recycling

Please contact Trajan for information regarding recycling purifier products.

### Information and support

Visit [www.trajanscimed.com](http://www.trajanscimed.com) or contact [techsupport@trajanscimed.com](mailto:techsupport@trajanscimed.com)

Specifications are subject to change without notice.

US AGENT	<b>Trajan Scientific Americas Inc</b>
	2601 Technology Drive,
	Louisville, KY 40299, USA
	Tel: +1 502 491 6300